

As⁺³

As⁺⁵

QUICK™

Rapid Arsenic Test Kit

Kit Part Number: 481396-5
5 Tests



Instruction Booklet	Page
About Kit #481396-5.....	2
Test Procedure.....	3
Instructions for Best Accuracy.....	4
Soil Test Procedure.....	5
Wood Test Procedure.....	5
Safety Data Sheets.....	6-7
Letter from the Kit Inventor.....	8

FOR BEST RESULTS, FOLLOW KIT INSTRUCTIONS.



WARNING:
Hydrogen and Arsine gases are generated during the test. Work in a well-ventilated area away from open flames and other sources of ignition. Review the Material Safety Data Sheet before handling any chemicals.

Industrial Test Systems, Inc.
1875 Langston Street, Rock Hill, SC 29730 USA
Phone: (800) 861-9712, (803) 329-9712, Fax: (803) 329-9743
Email: its@sensafe.com
ARSENICKITS.COM



ITS Europe, LTD
The UK Centre for Homeland Security
Building 7, Chilmark
Salisbury, Wiltshire SP3 5DU, UK
Phone: +44 (0)1722 717911
itseurope@sensafe.com

Information on the performance characteristics of Quick™ can be found at www.epa.gov/etv/verifications/verification-index.html, or call ITS at 803-329-9712 for a copy of the ETV verification report. The use of the ETV Name or Logo does not imply approval or certification of this product nor does it make any explicit or implied warranties or guarantees as to product performance.

ABOUT KIT # 481396-5:



Part Number: 481396-5, 5 Tests

Kit Components:

- 1 Reaction Bottle, clear PVC, with 20mL (lower), 50mL (middle), and 100mL (upper) lines
- 1 White Cap, with white turret, for holding test strip
- 5 Powder Pillows of First Reagent **1** (3.8 gm)
- 5 Powder Pillows of Second Reagent **2 MPS** (1 gm)
- 5 Powder Pillows of Third Reagent **3 ZINC** (2 gm)
- 5 Arsenic Test Strips in Foil Packets - **Caution:** Each test strip pad contains about 1 mg Mercuric Bromide (HgBr₂)
- This Instruction Booklet with MSDS
- 1 Yellow Cap for mixing
- Kit Box for Components
- Color Chart

This test detects soluble inorganic Arsenic (As⁺³ and As⁺⁵)


This Arsenic Test Kit provides a safe, simple, and reliable way to test for Arsenic from 0 to 0.5 mg/L (up to 2.5mg/L when using 1/5 dilution method). Follow the instructions carefully to get reliable results. All components are supplied in the kit except for a timer and thermometer. This test tolerates up to 2.0 mg/L Hydrogen Sulfide without interference. No interference was found for this test kit for Antimony up to 0.5mg/L. No interference from Iron or Sulfate was found. It is recommended that the water sample be 22°C - 28°C. The color chart was standardized at 24°C. For reference purposes, record the temperature at which the sample was run. Use all reagents and test strips within the allowed shelf life as marked on each container.

Chemistry of the Reaction (Modified Gutzeit method):

Inorganic Arsenic compounds in the water sample are converted to Arsine (AsH₃) gas by the reaction of Zinc Dust and Tartaric Acid. Ferrous and Nickel salts have been added to accelerate this reaction. The Arsine converts the Mercuric Bromide on the test strip to mixed Mercury halogens (such as AsH₃HgBr) that appear with a color change from white to yellow or brown. Potassium Peroxymonosulfate (second reagent) is added to oxidize Hydrogen Sulfide to Sulfate.

PRECAUTIONS: Hydrogen gas and Arsine gas are generated during the reaction. Work in a well-ventilated area away from fire and other sources of ignition. All reagents are unsuitable for human consumption.

US Patent # 6696300

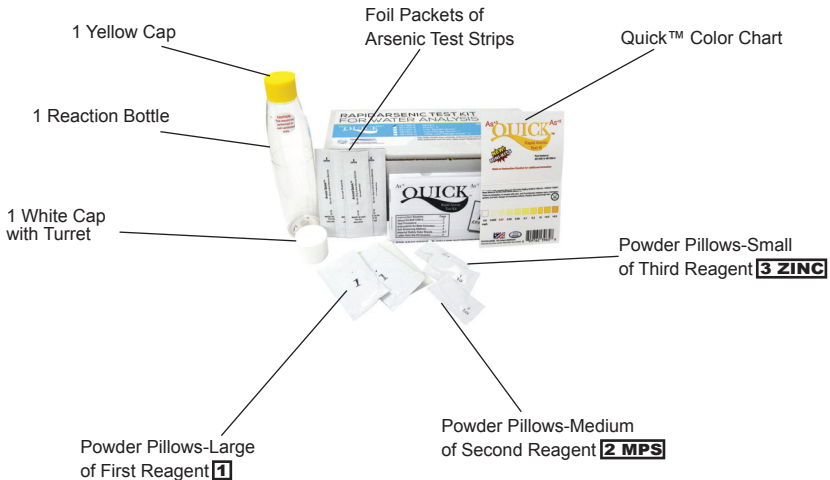

WARNING: Hydrogen and Arsine gases are generated during the test. Work in a well-ventilated area away from open flames and other sources of ignition. Review the Material Safety Data Sheet before handling any chemicals.



FOLLOW KIT INSTRUCTIONS CLOSELY.
Part Number: 481396-5, 5 Tests

Test Procedure:

1. For best results, the water temperature should be between 22°C to 28°C. Use a thermometer to verify the temperature of the sample.
2. To the Reaction Bottle, slowly add the water sample to the 100mL (upper) scored line on the bottle.
3. Add **1 Powder Pillow-Large** of First Reagent **1** to the Reaction Bottle. Cap the bottle securely with yellow mixing cap and shake vigorously for 15 seconds.
4. Uncap the Reaction Bottle; add **1 Powder Pillow-Medium** of Second Reagent **2 MPS**. Cap the bottle securely with yellow mixing cap and shake vigorously with bottle upright for 15 seconds. Allow the sample to sit for 2 minutes to minimize Sulfide interference.
5. Uncap the Reaction Bottle and add **1 Powder Pillow-Small** of Third Reagent **3 ZINC**. Cap the bottle securely with yellow mixing cap and shake vigorously for 5 seconds.
6. Remove yellow mixing cap. Recap the bottle immediately and securely using the white cap (must be dry) with turret up (open).
7. Remove one Arsenic test strip from the Arsenic Quick Foil Packet. In order for the results to be accurate, the test strip must be oriented correctly, and inserted to the correct depth. Insert the test strip into the turret as illustrated in Figure 2 and Figure 3:
 - a) Position the strip so that the test pad and red line are facing the back of the white cap (see Figure 2).
 - b) Insert the strip into the turret until the red line is even with the top of the turret, and close (flip down) the turret (see Figure 3). This will hold the test strip in place. (**Note: Steps 6 & 7 should be completed within 30 seconds.**)
8. Using a timer, allow the reaction to occur in an undisturbed, well-ventilated area for 10 minutes. Reaction generates small hydrogen gas bubbles.
9. After the 10 minute wait (but before 12 minutes), pull up the turret and carefully remove the test strip. Do not touch the reaction pad. Use the Quick™ Color Chart to match the reaction pad color. **COMPLETE MATCHING IMMEDIATELY (WAIT NO LONGER THAN 30 SECONDS)**. After 30 seconds have elapsed, the colors begin to change (yellow colors fade and browns turn grey or black). For best color matching results use natural daylight; avoid direct sunlight.
10. Record your result.

Note: To ensure complete transfer of reagent, shake or tap the packet before opening to move all reagent to the bottom of the packet.

(Mercuric Bromide strips (Arsenic test strips) will not react with arsine gas if they are wet)

ATTENTION: Soon after testing is completed, decant liquid from the bottle down a drain that is not used for food preparation and flush with water. Wet Zinc should be collected and disposed of according to local regulations. Rinse the bottle, white cap, and yellow cap with clean water. Shake off any excess water and dry the white cap with turret with a soft tissue. Drying the white turret cap is especially important if you plan to run the next test immediately. Store the used strips in the plastic bag marked "Used Mercuric Bromide (HgBr₂) Test Strips". Keep the used strips inaccessible to children and pets, and dispose according to local environmental regulations.



Figure 1



Figure 2





Figure 3

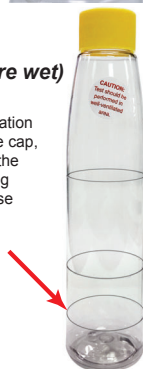

INSTRUCTIONS FOR BEST ACCURACY

1. To gain confidence in using this test kit for unknown samples, it is highly recommended that you use the kit on a sample with a known inorganic Arsenic concentration value, or with a sample that has been prepared using an Arsenic standard. By making a “practice run” of the test, you will familiarize yourself with all of the procedures necessary to ensure accurate testing results. Additionally, you will have the opportunity to become familiar with the process of color matching, which will help to ensure accurate test results. ITS suggests the test be run in duplicate for better accuracy.
2. The water sample must not be preserved with Nitric Acid or any other preservation method. Small amounts of strong acids will interfere with the test results; and therefore it is best that the water sample be freshly drawn and run within 8 hours. Water samples held for over 24 hours may read as much as 20% lower. The water sample should not contain any significant amount of buffers. If you are planning to send a duplicate sample for ICP laboratory verification, follow preservation requirements for that sample only.
3. The water and ambient temperature are very important to ensure accurate results. As an example, a water temperature of 15°C can result in the color development on the testing pad to be lighter than the actual Arsenic concentration in the tested sample (a false low reading occurs). When the water is cold, warm water sample to 22°C to 28°C before testing (using a microwave is acceptable). If the water temperature is above 28°C your result may read low (accelerator chemistry reacts too fast). Consideration must also be made for the air temperature when running the test. Best results are from 22°C to 28°C (water and air). The color chart and Arsenic Scan chart are calibrated at 24°C.
4. After the test has been run, try to rinse out the reaction bottle with clean tap water as soon as possible. When the reaction chemicals are allowed to sit in the reaction bottle after the reaction time, the zinc may begin to adhere to the bottom of the bottle. When this occurs, you may need to clean the reaction bottle with a bottlebrush. Another method for zinc removal is to use a 20% Hydrochloric Acid (reusable) rinse. Be sure to rinse the reaction bottle with clean tap water before running the next test.
5. When matching your test strip pad with the colors on the Easy-Read™ color chart, it may be helpful to find a color that is clearly lighter than the test strip pad and make note of it (as an example, we will use a value of 10 ppb). Next, find a color that is clearly darker than the test strip pad (as an example, we will use a value of 30 ppb). By defining a lowest and highest possible value range we can assume that the correct color match is 20 ppb. If the 20 ppb color matches, then you have determined your Arsenic level. In some cases, an exact color match will not be available. As an example, if your test strip pad is darker than 20 ppb and slightly lighter than 30 ppb, you can estimate a value 25 ppb as your result. Following these easy steps can make color matching more precise. Careful color matching will assure the best possible result.
6. Levels of Hydrogen Sulfide above 2 mg/L can interfere with this test, resulting in elevated Arsenic readings. Our test kit will eliminate up to 2 mg/L of Sulfide interference. There are two ways to overcome Hydrogen Sulfide levels above 2 mg/L: Allow the water sample to sit at room temperature, uncovered and exposed to air for 8 hours (about 50% of the H₂S gas dissipates for every 8 hours). Industrial Test Systems, Inc. sells Hydrogen Sulfide detection kits (part # 481197-20) for quick, accurate verification of this interfering ion. The test kit detects levels of 0.3, 0.5, 1.0, and 2.0 mg/L (ppm). The Hydrogen Sulfide test kit contains all components necessary to run the test, and is economically priced at \$15.99 for 30 tests.
7. Five tests can be run with each assembly. Do not use components from other kits. Interchanging components may result in inaccurate results since each kit is Quality Control released for accuracy with its given components. Three conditions can result in getting an incorrect reading: the presence of Hydrogen Sulfide above 2ppm; color matching in poor lighting conditions; and color blindness of operator.
8. It has been determined that irrigation of crops with arsenic water increases the soil arsenic levels which can increase the arsenic content in the crop. This Arsenic kit can be used for screening of Arsenic levels in soil. **See procedure on Page 5.**
9. If you have any questions or comments, please feel free to contact our R&D Department at 1-803-329-0162 ext 211 or by email at: its@sensafe.com.

SOIL TEST PROCEDURE

(Non-Digestion Method)

Scope and Application:

1. This method is valid for detection of Inorganic Arsenic in soil.
2. The minimum Arsenic detection with 0.5 g of soil is 1.0 mg/kg.

Sample Handling and Preparation (Recommended but not required):

3. Dry soil for at least 1 hour at 60°C or until completely dry.
4. Remove visible debris/stones from dried soil.
5. Grind the dried soil into a fine powder and mix until homogenous using a coffee grinder or a mortar and pestle.
(a Coffee Grinder works well)

Interferences:

6. Test tolerates up to 2 mg/kg of Hydrogen Sulfide, 9000 mg/kg of Iron, and 1500 mg/kg of Lead.

Test Procedure:

7. Weigh out 0.5 g of the dried soil and transfer to the Reaction Bottle supplied in the Arsenic Quick™ Kit (Part # 481396-5). Note: If the Sample Handling and Preparation steps are omitted, then use 1g of soil. One gram is used on assumption that soil is 50% moisture by weight.)
8. Fill the bottle to the 100mL (upper) scored line on the Reaction Bottle with Arsenic-free tap water or Distilled water.
9. Follow the standard test procedure for the Arsenic Quick™ Kit starting with Step 3 on page 3.

Calculation:

10. Multiply the test result by 300 (correction multiplier) to get the Arsenic concentration in the soil as mg Arsenic/kg Soil. (Example: 40 µg/L x 300 = 12 mg Arsenic/kg Soil)

NOTE: Because when compared to Acid Digestion/ICP-MS Arsenic analysis, this soil screening method gives typically 50% lower value; a correction multiplier of 300 is used (use 200 as a multiplier if you desire actual measured level).

NOTE: Advanced users can access the Acid Digestion/ICP-MS Arsenic analysis method at sensafe.com/quick-arsenic/.

WOOD TEST PROCEDURE

Ordinarily you could cut small wood splinters with a sharp knife from non-weathered wood to test for arsenic; however, since weathered wood will have the arsenic leached out from the surface, this technique would not get a representative wood sample. The older and more weathered the wood the deeper sample core of the wood is required. We recommend that you use a ¼" drill bit and a portable drill. Sampling the wood: Using a ¼" drill bit, drill a wood sample from an intact location on the wood. Usually a sample drilled ½" deep is adequate. If wood is older than 20 years you should drill about ¾" into the wood to get a good wood sample. Drill slowly into the wood, and simultaneously you should have a small, stiff cardboard (or any other convenient collector) below the drilling area to catch the drill dust generated by the drilling. Additional wood material will be generated as you pull out the drill from the core. This material must be added to the sample for testing. Carefully add all the wood drilled dust generated to the Reaction Bottle. You are ready to do the Arsenic Test.

1. Add wood chips (see procedure above) to the Reaction Bottle.
2. To the Reaction Bottle, slowly add the water sample to the 50mL (middle) scored line on the bottle.
3. Add **1 Powder Pillow** of First Reagent **1** to the Reaction Bottle.
4. Add **1 Powder Pillow** of Second Reagent **2 MPS** to the Reaction Bottle.
5. Cap bottle with yellow mixing cap and shake vigorously for 15 seconds to dissolve the reagents in the water.
6. Let the solution sit for 2 minutes, which **extracts arsenic** from wood.
7. Add **1 Powder Pillow** of Third Reagent **3 ZINC** to the reaction bottle.
Cap securely with the yellow mixing cap and shake vigorously for 5 seconds.
For best results, complete Steps 8 and 9 within the next 30 seconds.
8. Remove yellow mixing cap. Recap bottle securely using the white cap (must be dry) with turret up (open).
9. Remove one Arsenic test strip from the test strip foil packet. In order for the results to be accurate, the test strip must be oriented correctly, and inserted to the correct depth. Insert the test strip into the turret as illustrated in Figure 2 and Figure 3. Position the strip so that the test pad and red line are facing the back of the white cap (see Figure 2). Insert the strip into the turret until the red line is even with the top of the turret, and close (flip down) the turret (see Figure 3). This will hold the test strip in place.
10. Using a timer, allow the reaction to occur in an undisturbed, well ventilated area for 5 minutes. Reaction generates small hydrogen gas bubbles and arsine gas if arsenic is present.
11. After the 5 minute wait, pull up the turret and carefully remove the test strip. Do not touch the reaction pad. Observe the color of the test strip and determine arsenic concentration:

White indicates absence of arsenic (no arsenic).

Yellow indicates moderate amount of arsenic present (arsenic present).

Brown indicates high amount of arsenic present (arsenic present).

Complete color observation immediately (within 30 seconds).



SDS 1
Safety Data Sheet

Section 1 Product and Company Information

Product Name: First Reagent **Product Number:** 481196-D
Recommended use: Used to detect arsenic in water
Restricted use: Not applicable
Mfg. name: Industrial Test Systems, Inc.
Mfg. address: 1875 Langston Street, Rock Hill, SC
Emergency Telephone (poison control): 1-800-222-1222
Mfg. Telephone: 1-803-329-9712

Section 2 Hazard Identification

Hazard(s): Not hazardous: food grade tartaric acid, less than 1% of other ingredients.
Required labeling: Not applicable

Section 3 Composition/Information on Ingredients

Reagent	CAS	TSCA#	RTECS#	%	Hazard
L-Tartaric Acid	87-69-4	N/A	N/A	98.9	Food grade, N/A

Section 4 First-Aid Measures

Contact Area	First-aid
Eyes	Flush with large amounts of cold water for 15 minutes. Call a physician immediately.
Skin	Rinse with large amounts of water for 15 minutes. Remove contaminated clothing.
Ingestion	If swallowed, wash out mouth with water. Do not induce vomiting. Call a physician.
Inhalation	If inhaled, remove person to fresh air source. Call a physician.
Most likely effect	Irritation of skin and nose.

Section 5 Fire Fighting Measures

Extinguishing media: Use that which is appropriate for the surrounding fire.
Explosion Hazard: Not flammable or combustible.
Flash Point: N/A **Special fire fighting procedures:** N/A

Section 6 Accidental Release Measures

Sweep up and dispose in normal trash. Do not breathe dust. Wash hands.

Section 7 Handling and Storage

Use standard hygienic practices (no eating, drinking, or smoking) around the product. Wash hands after use. Keep away from children and pets. Keep container tightly closed. Use in well ventilated area. Handle carefully to limit dust.

Section 8 Exposures Controls/Personal Protection

OSHA Permissible Limits: No data
Engineering controls: Adequate ventilation. Use dust mask if there is a large spill.
Personal Protective Equipment (PPE): Use PPE appropriate for the surroundings.
Other: Use gloves to prevent contact irritation. Use eye protection to prevent droplets from entering the eye. Ensure an eyewash station is available.

Section 9 Physical and Chemical Properties

Appearance: White, granular free-flowing solid **Melting/Freezing point:** N/A
Decomposition temperature: No data **Upper/Lower flammability limit:** No data
Solubility: Water soluble **Viscosity:** N/A **Odor:** odorless
Initial boiling point/range: N/A **Vapor Pressure:** Not volatile
Flash point: No data **Odor threshold:** N/A **Evaporation rate:** N/A
Vapor density: N/A **Flammability:** flammable **pH:** Acidic
Partition coefficient: N/A **Relative density:** No data
Auto-ignition temperature: No data

Section 10 Stability and Reactivity

Product is stable under normal conditions. Hazardous polymerization will not occur. Reacts with zinc, silver, and/or aluminum in the presence of water or moisture to rapidly release explosive hydrogen gas.

Section 11 Toxicological Information

No data. Do not breathe dust.

Section 12 Ecological Information

Data not available.

Section 13 Disposal Considerations

Dispose in normal trash. Do not breathe dust. At no time should First Reagent, Second Reagent, and Third Reagent be mixed together in dry (powder) form!

Section 14 Transport Considerations

Not applicable - material is not hazardous

Section 15 Regulatory Information

The above information is believed to be correct but does not purport to be all-inclusive and shall be used ONLY as a guide. Keep away from children and pets. Store in a dry, cool place. Keep container tightly closed.

Section 16 Other Information

Preparer: H. R.
Date Prepared: 5-3-17
Supersedes Revision: 10-10-16
Disclaimer: The information in this Safety Data Sheet is accurate to the best of our knowledge. It is designed only as a guidance for safe use, handling, storage, and disposal. This information is not considered to be a warranty or a quality specification.

SDS 1
Safety Data Sheet

Section 1 Product and Company Information

Product Name: Second Reagent **Product Number:** 481196-E
Recommended use: Used to detect arsenic in water
Restricted use: Not applicable
Mfg. name: Industrial Test Systems, Inc.
Mfg. address: 1875 Langston Street, Rock Hill, SC
Emergency Telephone (poison control): 1-800-222-1222
Mfg. Telephone: 1-803-329-9712

Section 2 Hazard Identification

Hazard(s): DANGER: CORROSIVE. Causes skin and eye damage. May be fatal if swallowed. Irritation to nose and throat.

Required labeling: N/A

Section 3 Composition/Information on Ingredients

Reagent	CAS	TSCA#	RTECS#	%	Hazard
Potassium Peroxymonosulfate	10058-23-8	N/A	N/A	N/A	%: 43 Hazard: N/A
Potassium Bisulfate	7646-93-7	N/A	N/A	N/A	%: 23 Hazard: N/A
Potassium Sulfate	7778-80-5	N/A	N/A	N/A	%: 29 Hazard: N/A
Potassium Peroxydisulfate	7727-21-1	N/A	N/A	N/A	%: 3 Hazard: N/A
Magnesium Carbonate	546-93-0	N/A	N/A	N/A	%: 2 Hazard: N/A

Section 4 First-Aid Measures

Contact Area	First-aid
Eyes	Flush with large amounts of cold water for 15 minutes.
Skin	Rinse with large amounts of water for 15 minutes. Remove contaminated clothing.
Ingestion	If swallowed, do not induce vomiting. Drink 1-2 glasses of water to dilute the stomach contents. Do not give water to the victim if they are unconscious. Call a physician immediately.
Inhalation	If inhaled, remove person to fresh air source. If breathing is still difficult, have a trained person administer oxygen. If not breathing, give artificial respiration. Call a physician immediately.

Most likely effect: Irritation

Section 5 Fire Fighting Measures

Extinguishing media: Water **Explosion Hazard:** Not flammable or combustible. Will release oxygen when heated, acid mist may be present **Flash Point:** N/A
Special fire fighting procedures: N/A

Section 6 Accidental Release Measures

Sweep up and dispose in normal trash. Do not breathe dust. Wash hands.

Section 7 Handling and Storage

Use standard hygienic practices (no eating, drinking, or smoking) around the product. Wash hands after use. Keep away from children and pets. Keep container tightly closed. Mixing with compounds containing halides or active halogens can cause release of the respective halogen in the presence of moisture. Mixing with cyanides can cause release of hydrogen gas. Mixing with heavy metal salts such as those of cobalt, nickel, copper, or manganese can cause decomposition with release of oxygen and heat.

Section 8 Exposures Controls/Personal Protection

OSHA Permissible Limits: No data **Engineering controls:** Adequate ventilation. Use dust mask if there is a large spill. **Personal Protective Equipment (PPE):** Use PPE appropriate for the surroundings. **Other:** Use gloves to prevent contact irritation. Use eye protection to prevent droplets from entering the eye. Ensure an eyewash station is available.

Section 9 Physical and Chemical Properties

Appearance: White, granular free-flowing solid **Melting/Freezing point:** N/A
Decomposition temperature: No data **Upper/Lower flammability limit:** No data
Solubility: N/A **Viscosity:** N/A **Odor:** odorless **Initial boiling point/range:** N/A
Vapor Pressure: Not volatile **Flash point:** No data **Odor threshold:** N/A
Evaporation rate: N/A **Vapor density:** N/A **Flammability:** flammable
pH: 2.3 (1% in water) **Partition coefficient:** N/A **Relative density:** 1.1 – 1.4
Auto-ignition temperature: No data

Section 10 Stability and Reactivity

Product is stable under normal conditions. Hazardous polymerization will not occur. Reacts with zinc, silver, and/or aluminum in the presence of water or moisture to rapidly release explosive hydrogen gas.

Section 11 Toxicological Information

Acute Effects:

- Skin Absorption: >11,000 mg/kg (rabbits)
- Oral LD₅₀: 2,000 mg/kg (rats)
- Inhalation LC₅₀: >5 mg/L (rats) (4 hour)

Section 12 Ecological Information

Data not available.

Section 13 Disposal Considerations

Dispose in normal trash. Do not breathe dust. At no time should First Reagent, Second Reagent, and Third Reagent be mixed together in dry (powder) form!

Section 14 Transport Considerations

Not applicable - material is not hazardous

Section 15 Regulatory Information

The above information is believed to be correct but does not purport to be all-inclusive and shall be used ONLY as a guide. Keep away from children and pets. Store in a dry, cool place. Keep container tightly closed.

Section 16 Other Information

Preparer: H. R. **Date Prepared:** 5-3-17 **Supersedes Revision:** 12-16-15
Disclaimer: The information in this Safety Data Sheet is accurate to the best of our knowledge. It is designed only as a guidance for safe use, handling, storage, and disposal. This information is not considered to be a warranty or a quality specification.

SDS 1
Safety Data Sheet

Section 1 Product and Company Information

Product Name: Third Reagent **Product Number:** 481196-E
Recommended use: Used to detect arsenic in water
Restricted use: Not applicable
Mfg. name: Industrial Test Systems, Inc.
Mfg. address: 1875 Langston Street, Rock Hill, SC
Emergency Telephone (poison control): 1-800-222-1222
Mfg. Telephone: 1-803-329-9712

Section 2 Hazard Identification

Hazard(s): TOXIC: May be fatal if swallowed. IRRITANT: Irritation to nose and throat.
Required labeling: Not applicable

Section 3 Composition/Information on Ingredients

Reagent	CAS	TSCA#	RTECS#	%	Hazard
Zinc	7440-66-6	N/A	N/A	>99	Toxic, irritant

Section 4 First-Aid Measures

Contact Area	First-aid
Eyes	Flush with large amounts of cold water for 15 minutes. Call a physician immediately.
Skin	Wash with soap and water for 15 minutes. Remove contaminated clothing.
Ingestion	If swallowed, wash out mouth with water. If a large amount is swallowed, call a physician. Antidote: Calcium disodium edetate/dextrose, intravenous; Calcium disodium edetate/procaine, intramuscular.
Inhalation	If inhaled, remove person to fresh air source. Call a physician.
Most likely effect	Irritation of skin and nose.

Section 5 Fire Fighting Measures

Extinguishing media: Dry chemical, sand, lime, soda ash.
Explosion Hazard: Very fine dust may form explosive mixtures with air.
Flash Point: N/A **Special fire fighting procedures:** Do not use water or foam

Section 6 Accidental Release Measures

Do not touch spilled material. Avoid heat, flames, sparks, and other sources of ignition. Remove sources of ignition. Collect material into suitable, loosely covered container for disposal. Do not get water directly on material.

Section 7 Handling and Storage

Use standard hygienic practices (no eating, drinking, or smoking) around the product. Wash hands after use. Keep away from children and pets. Keep container tightly closed. Use in well ventilated area. Handle carefully to limit dust. Store in a cool, dry place.

Section 8 Exposures Controls/Personal Protection

OSHA Permissible Limits: N/A
Engineering controls: Adequate ventilation. Use dust mask if there is a large spill.
Personal Protective Equipment (PPE): Use PPE appropriate for the surroundings.
Other: Use gloves to prevent contact irritation. Use eye protection to prevent droplets from entering the eye. Ensure an eyewash station is available.

Section 9 Physical and Chemical Properties

Appearance: Grayish, powdery solid **Melting/Freezing point:** 420°C/N/A
Decomposition temperature: No data **Upper/Lower flammability limit:** No data
Solubility: reacts **Viscosity:** N/A **Odor:** odorless
Initial boiling point/range: N/A **Vapor Pressure:** 1 mmHg @ 487°C
Flash point: No data **Odor threshold:** N/A **Evaporation rate:** N/A
Vapor density: N/A **Flammability:** flammable **pH:** N/A
Partition coefficient: N/A **Relative density:** 7.14
Auto-ignition temperature: No data

Section 10 Stability and Reactivity

Product is stable under normal conditions. Hazardous polymerization will not occur. Finely divided powder may react with water. Keep away from acids, bases, metals, oxidizers, reducing agents, combustible materials.

Section 11 Toxicological Information

Eye Contact: Dust may cause mechanical irritation or injury to the surface of the eye, with discomfort, reddening, and tearing. Direct contact may cause serious corneal burns.
Skin Contact: Dust may cause mechanical irritation and mild dermatitis.
Ingestion: Large oral doses may cause gastrointestinal distress with stomach cramps, dehydration, electrolyte imbalance, abdominal pain, nausea, vomiting, hematemesis, diarrhea, lethargy, immune system effects, fever, dizziness, tightness in the throat, shock, collapse, renal failure, and death.

Section 12 Ecological Information

Data not available.

Section 13 Disposal Considerations

Dispose in normal trash. Do not breathe dust. At no time should First Reagent, Second Reagent, and Third Reagent be mixed together in dry (powder) form!

Section 14 Transport Considerations

Not applicable - packaged as part of a reagent set.

Section 15 Regulatory Information

The above information is believed to be correct but does not purport to be all-inclusive and shall be used ONLY as a guide. Keep away from children and pets. Store in a dry, cool place. Keep container tightly closed.

Section 16 Other Information

Preparer: H. R.
Date Prepared: 10-10-16
Supersedes Revision: 12-16-15
Disclaimer: The information in this Safety Data Sheet is accurate to the best of our knowledge. It is designed only as a guidance for safe use, handling, storage, and disposal. This information is not considered to be a warranty or a quality specification. This company shall not be held liable for any damage resulting from handling or from contact with the above product.

SDS 1
Safety Data Sheet

Section 1 Product and Company Information

Product Name: Arsenic Quick Strip **Product Number:** 481196-G
Recommended use: Used to detect arsenic in water
Restricted use: Not applicable
Mfg. name: Industrial Test Systems, Inc.
Mfg. address: 1875 Langston Street, Rock Hill, SC
Emergency Telephone (poison control): 1-800-222-1222
Mfg. Telephone: 1-803-329-9712

Section 2 Hazard Identification

Hazard(s): Pad contains Mercury.
Required labeling: N/A

Section 3 Composition/Information on Ingredients

Reagent: Mercuric Bromide **CAS:** 7789-47-1 **TSCA#:** N/A
RTECS#: OV7415000 **%:** Approx. 1mg **Hazard:** Oral LD₅₀ (rat) 40mg/kg

Section 4 First-Aid Measures

Contact Area	First-aid
Eyes	Flush with copious amounts of cold water for 5 minutes.
Skin	Rinse with large amounts of water for 2 minutes. Remove contaminated clothing.
Ingestion	Rinse mouth with water. As a precaution, call a physician or Poison Control.
Inhalation	Evacuate to fresh air. If breathing is difficult, give oxygen and seek medical advice.
Most likely effect	Irritation

Section 5 Fire Fighting Measures

Extinguishing media: Use that which is appropriate for the surrounding fire.
Explosion Hazard: None found **Flash Point:** N/A
Special fire fighting procedures: N/A

Section 6 Accidental Release Measures

Sweep up strips and put into a plastic bag labeled "Used Test Strips." Dispose of used strips per local environmental and regulatory requirements. Wash hands after use.

Section 7 Handling and Storage

Use standard hygienic practices (no eating, drinking, or smoking) around the product. Wash hands after use. Keep away from children and pets. Keep container tightly closed.

Section 8 Exposures Controls/Personal Protection

OSHA Permissible Limits: N/A **Engineering controls:** N/A
Personal Protective Equipment (PPE): Use PPE appropriate for the surroundings.
Other: Use gloves to prevent contact irritation. Use eye protection to prevent droplets from entering the eye. Ensure an eyewash station is available.

Section 9 Physical and Chemical Properties

Appearance: Off-white pad on plastic handle **Melting/Freezing point:** N/A
Decomposition temperature: No data **Upper/Lower flammability limit:** No data
Solubility: N/A **Viscosity:** N/A **Odor:** odorless **Initial boiling point/range:** N/A
Vapor Pressure: N/A **Flash point:** No data **Odor threshold:** N/A
Evaporation rate: N/A **Vapor density:** N/A **Flammability:** flammable
pH: N/A **Partition coefficient:** N/A **Relative density:** N/A
Auto-ignition temperature: No data

Section 10 Stability and Reactivity

Product is stable. Hazardous polymerization will not occur. Firefighters should wear full protective clothing and self-contained breathing apparatus when fighting fires involving plastic and PVC materials.

Section 11 Toxicological Information

Each strip contains about 1mg Mercuric Bromide so toxicological effects are minimal because of the low exposure. Material, however, is toxic and should be handled carefully to minimize exposure. Place all used test strips into a plastic bag labeled "Used Test Strips." Dispose of used strips per local environmental and regulatory requirements. Wash hands after use.

Section 12 Ecological Information

Data not available.

Section 13 Disposal Considerations

Dispose of the test strips according to regulatory requirements.

Section 14 Transport Considerations

Not applicable - the strips are not hazardous

Section 15 Regulatory Information

This strip is considered an article under OSHA rules (CFR29, 1910.1200). *Article means a manufactured item other than a fluid or particle: (i) which is formed to a specific shape or design during manufacture; (ii) which has end use function(s) dependent in whole or in part upon its shape or design during end use; and (iii) which under normal conditions of use does not release more than very small quantities, e.g., minute or trace amounts of a hazardous chemical (as determined under paragraph (d) of this section), and does not pose a physical hazard or health risk to employees*.

A Safety Data Sheet (SDS) is not required for articles. This SDS is provided as a courtesy.

Section 16 Other Information

Preparer: H. R. **Date Prepared:** 5-3-17 **Supersedes Revision:** 9-21-16
Disclaimer: The information in this Safety Data Sheet is accurate to the best of our knowledge. It is designed only as a guidance for safe use, handling, storage, and disposal. This information is not considered to be a warranty or a quality specification.


Our products are compliant with all
49CFR and IATA rules and regulations.

LETTER FROM THE KIT INVENTOR

Thank you for purchasing our U.S. Patented (# 6,696,300) Arsenic Quick™ II Kit. Our company has trademarked the kits Quick™ because of the short 14 minute time for analysis.

The Drinking Water standard of the US EPA and the World Health Organization (WHO) allows a maximum contaminant level of 10 ppb (µg/L) for Arsenic. The old US EPA level of 50 ppb (µg/L) remains as the maximum contaminant level for many countries in the world.


For several years, Industrial Test Systems, Inc. (ITS) committed a major research & development effort to provide better and safer arsenic test kits. The goal was achieved. The test was made safer by using tartaric acid, instead of strong acids, for the reduction of inorganic arsenic (As⁺³/As⁺⁵) to arsine gas. For these efforts a US Patent was granted for the acceleration of the arsenic detection chemistry by the addition of metal enhancers, iron and nickel salts. This permits Arsenic field tests to be completed faster. The Quick™ II series of kits use a modified Turret cap which allows detection of arsenic below 10 ppb (µg/L). The reduction reactions utilized in all kits are as follows:



The analysis is performed in a closed reaction bottle (plastic) with an appropriate volume of sample (50 to 500 ml). After the 10 minute reduction reaction, the mercuric bromide strip or testing pad is removed and matched to the color chart or color analyzed by the Quick™ Arsenic Scan instrument. A light yellow to brown color change indicates that arsenic is present. The color intensity is proportionately related to the concentration of arsenic in the sample. NOTE: ITS test kits detect free inorganic arsenic only. ICP-MS methods detect inorganic and organic arsenic. If organic arsenic is present, ITS kit results can be expected to give lower values when compared to ICP-MS results.

Quick™ Arsenic Test Kits Available:

US Patent # 6696300

PRODUCT NAME (PART NUMBER)	NO. OF TESTS		OPTIMUM RANGE* ppb (µg/L)	TYPICAL COLOR CHART DETECTION LEVELS ppb (µg/L)	TYPICAL ACCURACY** OF DUPLICATES USING QUICK™ ARSENIC SCAN
Arsenic Quick™ Mini Kit (481396-5) <small>(Can be used for soil & wood analysis)</small>	5	YES	10 to 200	0, 5, 10, 20, 60, 100, 300, 500, >500, >>500	+/-18 ppb or +/-30%
Arsenic Quick™ II Mini Kit (481303-5)	5	YES	3 to 20	<1, 2, 3, 4, 5, 6, 7, 8, 10, 13, 20, 25, 30, 40, >50, >80, >120, >160	+/-1.2 ppb or +/-16%
Arsenic Low Range Quick™ II Mini Kit (481301-5)	5	YES	1 to 10	<0.5, 1, 1.5, 2, 3, 4, 5, 6, 7, 8, 12, >20, >30, >50	+/-0.8 ppb or +/-14%
Arsenic Ultra-Low Quick™ II Mini Kit (481300-5)	5	YES	0.5 to 6	0, 0.3, 0.7, 1.0, 1.5, 2, 2.5, 3, 3.5, 4, 5, 6, 8, 10, 13, 20, >20	+/-0.4 ppb or +/-12%
Arsenic Quick™ Kit (481396) <small>(Can be used for soil & wood analysis)</small>	100	YES	10 to 200	5, 10, 20, 30, 40, 50, 60, 80, 100, 150, 200, 250, 300, 400, 500, >500	+/-18 ppb or +/-30%
Arsenic Low Range Quick™ (481297-I)	50	YES	7 to 80	<2, 4, 10, 15, 20, 25, 30, 40, 50, 60, 70, 80, 100, >150, >300	+/-8 ppb or +/-25%
Arsenic Quick™ II (481303)	50	YES	3 to 20	<1, 2, 3, 4, 5, 6, 7, 8, 10, 13, 20, 25, 30, 40, >50, >80, >120, >160	+/-1.2 ppb or +/-16%
Arsenic Low Range Quick™ II (481301)	50	YES	1 to 10	<0.5, 1, 1.5, 2, 3, 4, 5, 6, 7, 8, 12, >20, >30, >50	+/-0.8 ppb or +/-14%
Arsenic Ultra-Low Quick™ II (481300)	25	YES	0.5 to 6	0, 0.3, 0.7, 1.0, 1.5, 2, 2.5, 3, 3.5, 4, 5, 6, 8, 10, 13, 20, >20	+/-0.4 ppb or +/-12%
Quick™ Arsenic Scan Instrument (481305)	1 meter	YES	N/A	0.01 to >1.00 color density ppb (µg/L) <small>(as low as 0.2 ppb (µg/L) arsenic)</small>	(see above)

Information on the performance characteristics of Quick™ can be found at www.epa.gov/etv, or call ITS at 1-800-861-9712 for a copy of the ETV verification report. The use of the ETV® Name and Logo does not imply approval or certification of this product nor does it make any explicit or implied warranties or guarantees as to product performance.

*Optimum range is dependent on the sample matrix. **Typical accuracy listed is from data generated by a technician in our lab using the Quick™ Arsenic Scan instrument measuring reference free aqueous arsenic standards. All expected accuracy is in the larger of the two values listed. Example using Quick™ II: If the mean is 41 ppb, then the typical accuracy is +/-18 ppb which is larger than +/-12 ppb (40 ppb x 30%).

Where precision is important, ITS recommends that you run the water sample in duplicate, since the typical color matching is within one color block. For best precision consider the purchase of our Quick™ Arsenic Scan instrument. This unit is ideal for use with all test kits. Please contact our sales department at 803-329-9712 for more information or to order the Quick™ Arsenic Scan instrument.

Typical shelf life of kits is over 12 months. The kit includes First Reagent (Tartaric acid with iron and nickel salts); Second Reagent (MPS, an oxidizer); Third Reagent (zinc dust); and mercuric bromide strips, which contains about 1mg mercury per strip. After use, the strips should be discarded according to local environmental regulations. The Second Reagent must not be shipped by passenger airlines. Valuable information about the kit is in the MSDS literature. As a safeguard to minimize the operator's exposure to arsine and hydrogen gas, please run all tests in a well-ventilated area away from open flames and other sources of ignition. Arsine gas is highly toxic; and this precaution becomes more urgent if the water sample has high arsenic levels.

Cordially yours,

Ivars Jaunakais, Analytical Chemist
email: Ivars@sensafe.com